
# INSTRULYSE

## LOW ALKALINE DISINFECTING DETERGENT FOR PRE-DISINFECTION OF MEDICAL DEVICES

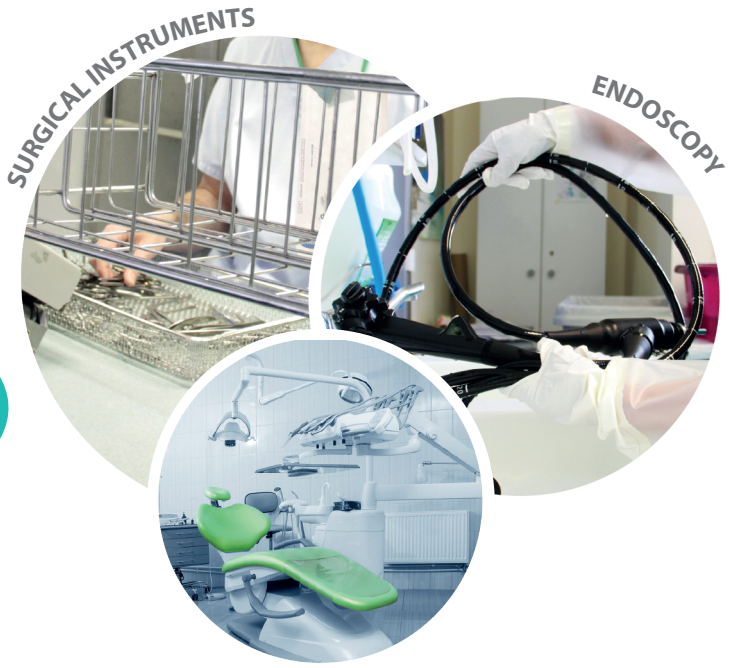


### AREAS OF APPLICATION

- Operating room, endoscopy, liberal medecine

QUATERNARY AMMONIUM FREE

### PRODUCT ADVANTAGES

- Quaternary ammonium free, phosphate or derivatives free, EDTA free and CMR* free
- Control of corrosion risks even in hard water condition.
- Can be used in an ultrasonic cleaner
- Ultra-concentrated formulation: 5L = 1250L of active solution

** Cancerigen, Mutagen substance toxic for Reproduction*




Franklab®
notre expertise l'Ultra-Propreté

MANUAL TREATMENT

DILUTION 0,4%

CE 0459

www.steririfrance.com

# INSTRULYSE

## LOW ALKALINE DISINFECTING DETERGENT FOR PRE-DISINFECTION OF MEDICAL DEVICES

## INSTRUCTIONS FOR USE

### Preparation of the solution at 0,4% :

- Wear suitable personal protective equipment (see Safety Data sheet)
- Dilute 20 ml of **INSTRULYSE** in 5L of water and homogenize the solution

### Use :

**1-** Fully immerse the soiled medical devices in the bath
**2-** Scrub the medical devices and use a swab if necessary
**3-** Contact time : 15 minutes
**4-** Rinse thoroughly with water
*Renew the bath for each use (or follow local recommendations)*

## DISINFECTING PROPERTIES

| Activity | Standards | Concentration | Contact time |
|---|---|---|---|
| **Bactericidal** | EN 13727 | 0,4% | 15 minutes |
| | EN 14561 | 0,4% | 15 minutes |
| **Yeasticidal** | EN 13624 | 0,4% | 15 minutes |
| | EN 14562 | 0,4% | 15 minutes |
| **Virucidal** | EN 14476<br>*Virus PRV (hepatitis B model), Virus BVDV (hepatitis C model),* | 0,4% | 15 minutes |
| | EN 17111<br>*Vaccinia Virus* | 0,4% | 15 minutes |

## PRECAUTIONS OF USE

See (SDS120)

## FEATURES

- Form : **Liquid**
- pH at 0,4% : **9**
- Color : **colorless to yellow, orange**

## COMPOSITION

- Alkylamine
- Non-ionic surfactants
- Easily biodegradable sequestrants
- Excipients

## PACKAGING

❶ Box of 500 doses of 20 ml.....réf. **12010**
❷ Box of 12x1 L.....réf. **12040**
❸ Box of 4 x 5 L.....réf. **12050SP**




Hazardous product - Follow precautions of use. Always read label and product information before use. Class IIb Medical device.

Document non contractuel - Imprimé en France

Franklab®
notre expertise l'Ultra-Propreté

3 av. des Frênes 78180 MONTIGNY LE BRETONNEUX ■ France
Tél. : **+ 33 (0)1 39 44 93 40** ■ Fax : **+ 33 (0)1 39 44 93 41**
**contact@sterifrance.com** ■ **www.sterifrance.com**

**FT 1890**
v4_07.2021